

Quantification of luminescence inhibition on TLC plates

Wolfgang Schulz, Wolfram Seitz, and Walter H. Weber

Objectives

- Development of an algorithm for evaluation of luminescence inhibition on TLC plates
- Comparison of TLC plate test with classic cuvette test
- Application in water analysis

Conclusions

- Sensitivity of luminescence inhibition test on TLC plate was found to be very high compared to cuvette test
- New luminescence inhibition was detected in treated process waste waters using TLC test


Method comparison

Luminescent inhibition test on TLC plates

- Application of substance onto silica gel plates
- Submerging into bacteria suspension
- Taking a picture After the Incubation time of 10 min
- Determination of the Inhibition values by a special software.

Luminescent inhibition cuvette test


- Sample + 2 % NaCl
- Addition of bacteria suspension
- Incubation time of 30 min at 15 °C (LUMIStherm)
- Detection (LUMIStox 300)

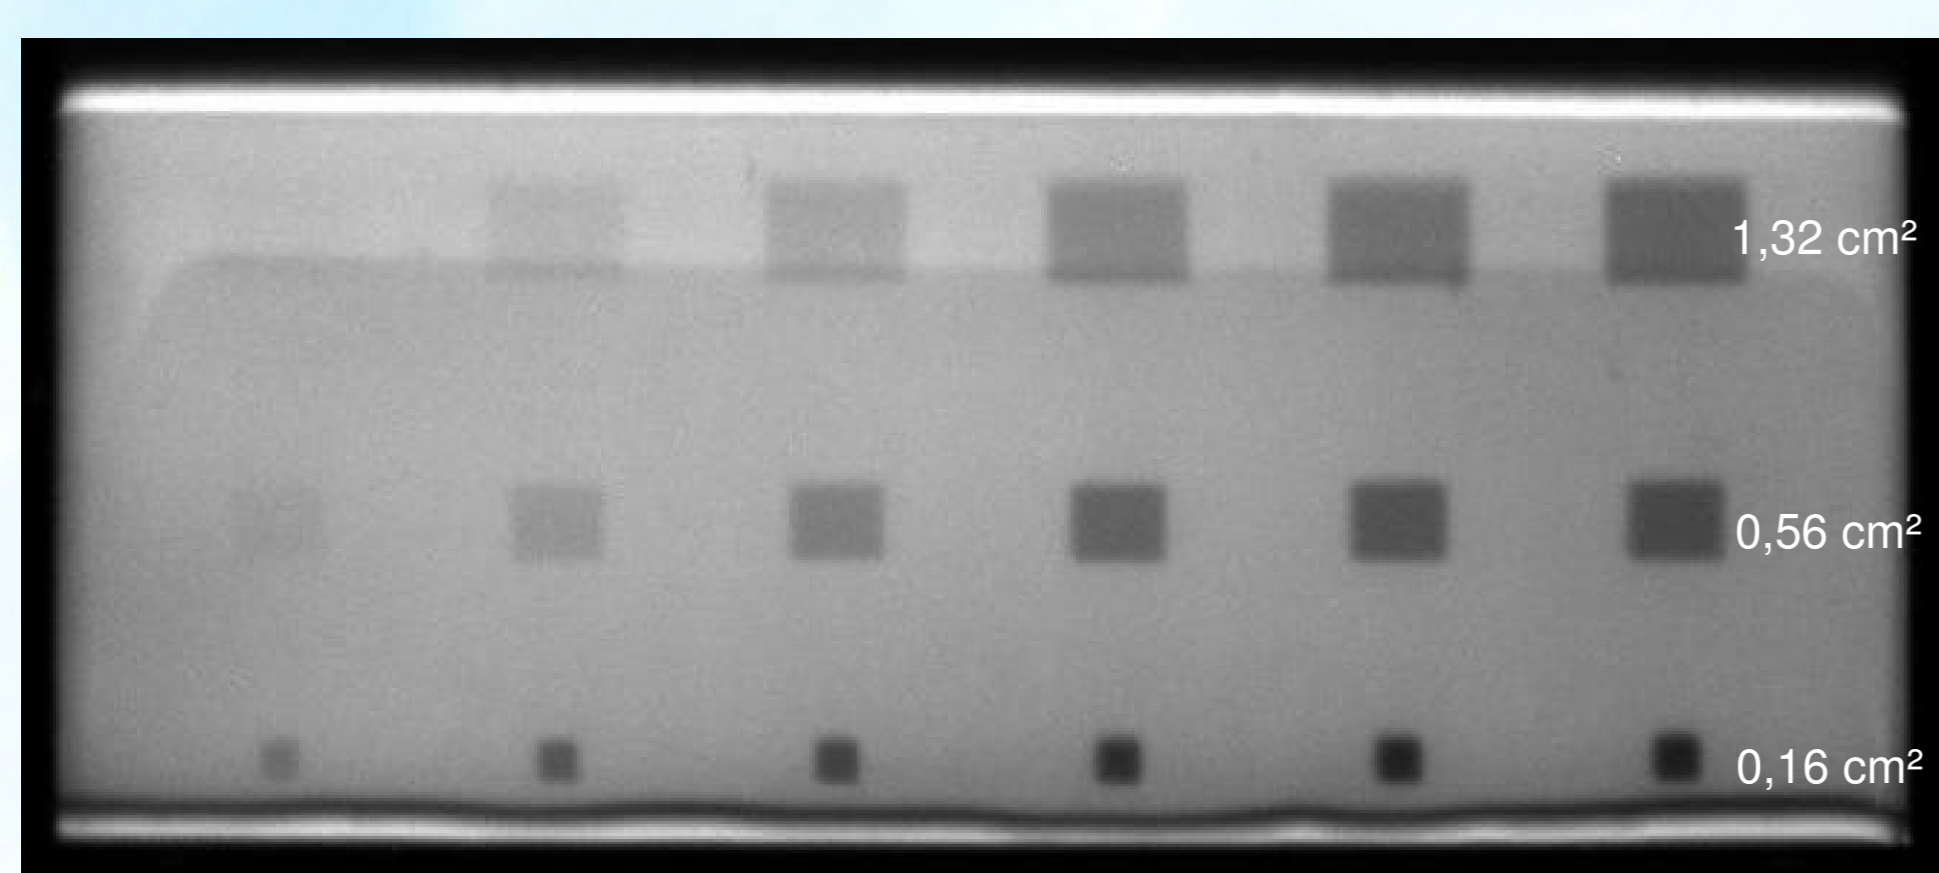


$$I^S = 1 - \frac{\sum_{n_1}^{n_2} i_n^S}{\sum_{n_1}^{n_2} i_n^S}$$





(1) LUMIStox 300
(2) LUMIStherm

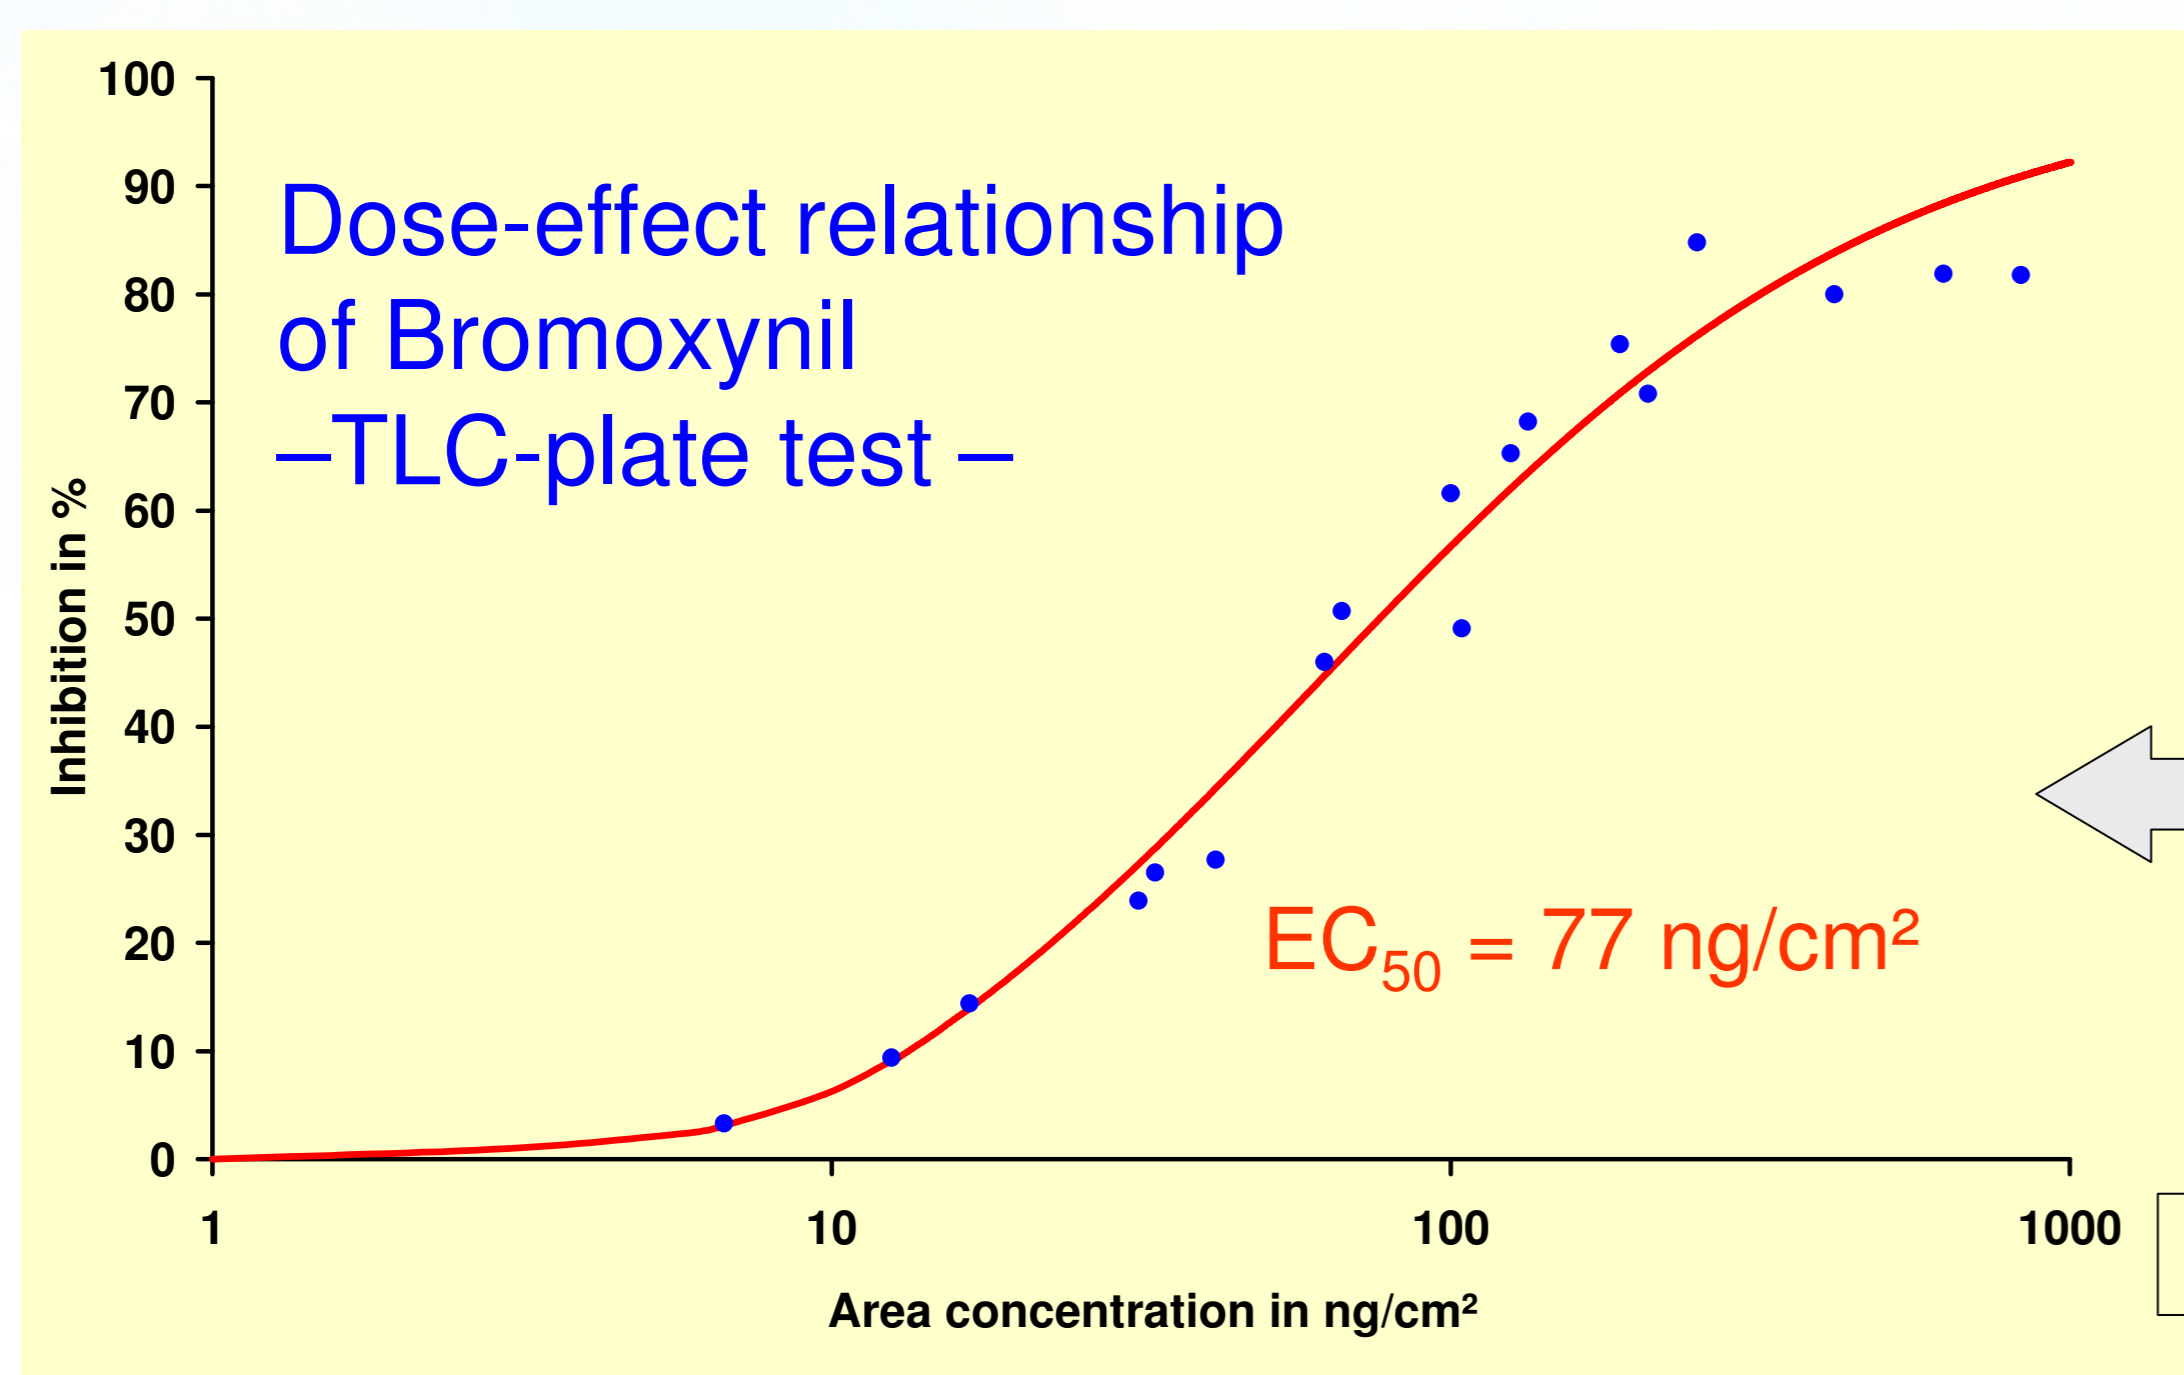

I = Inhibition
S = Sample
i = Intensity
n = Pixel number

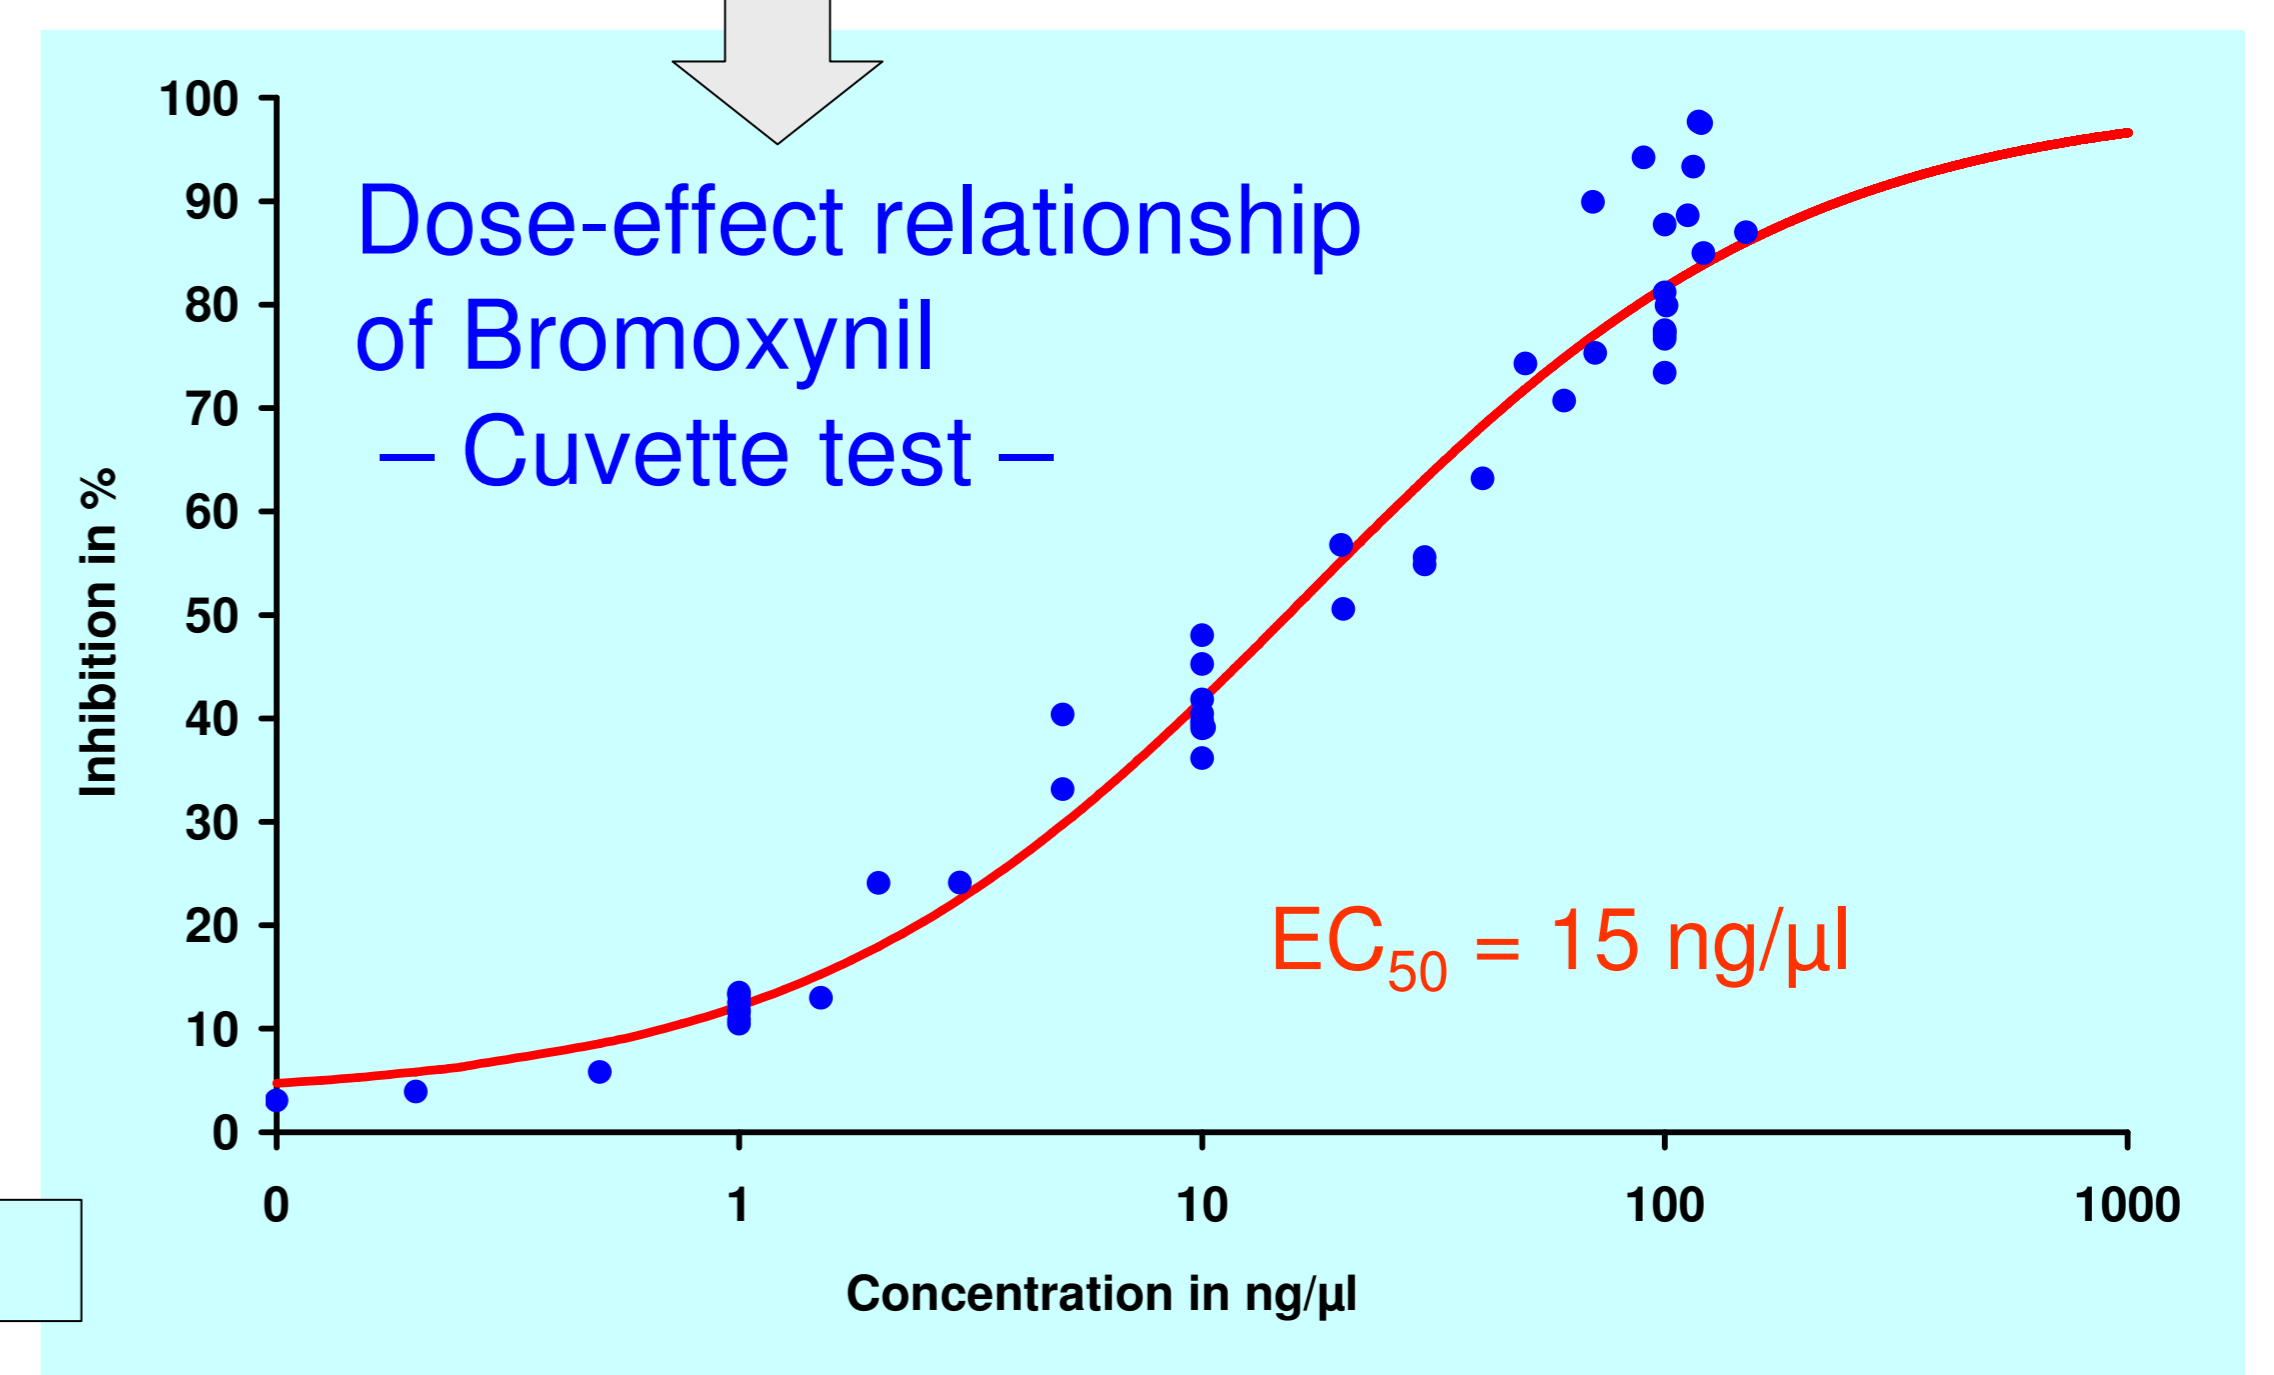

Sensitivity of TLC test is increased by a factor (F) of 1440 for pesticide Bromoxynil

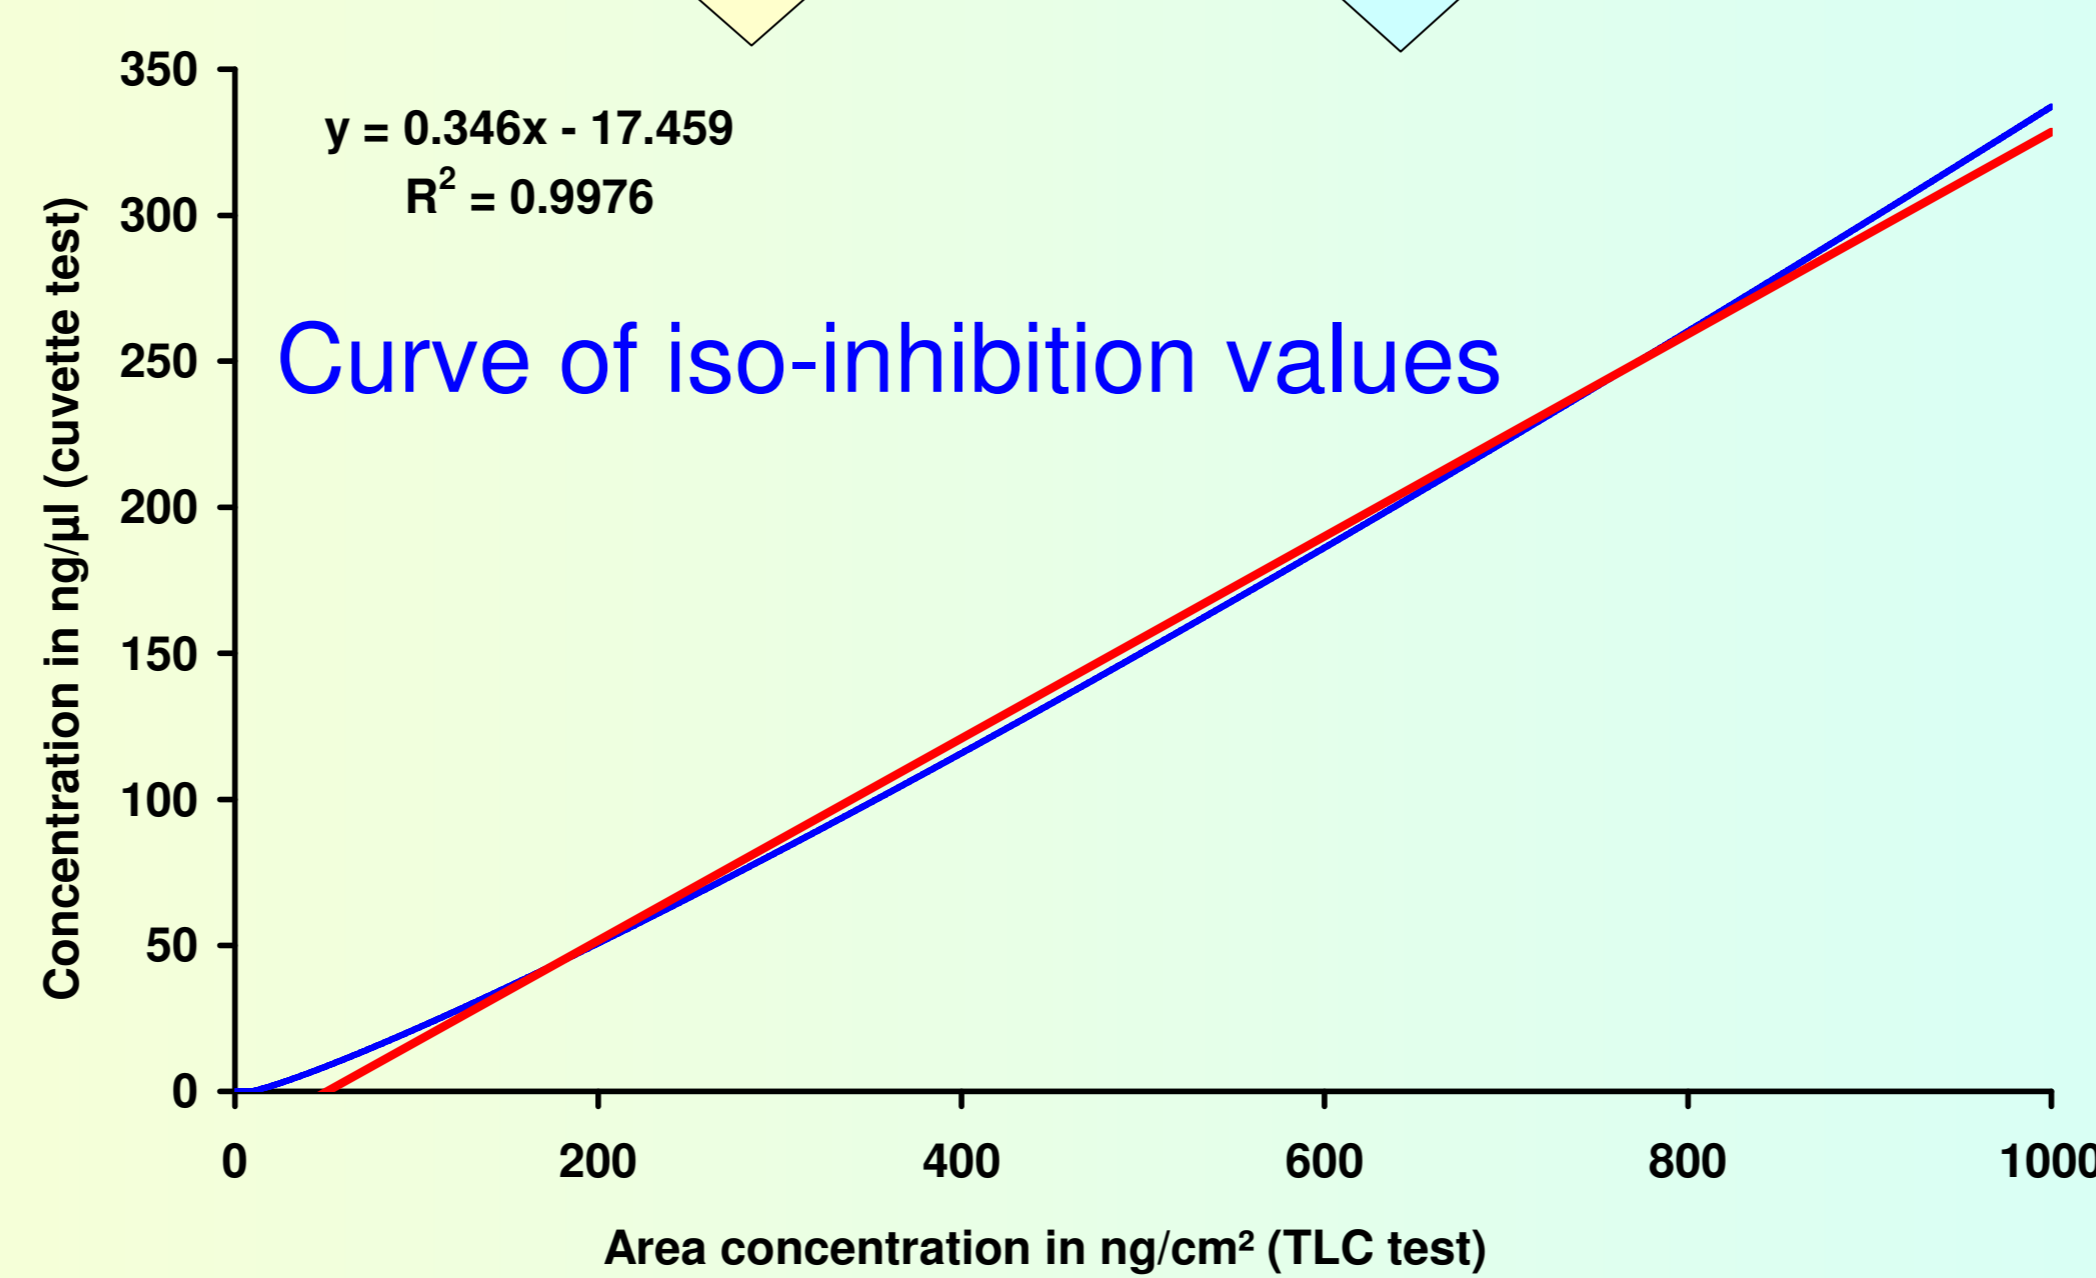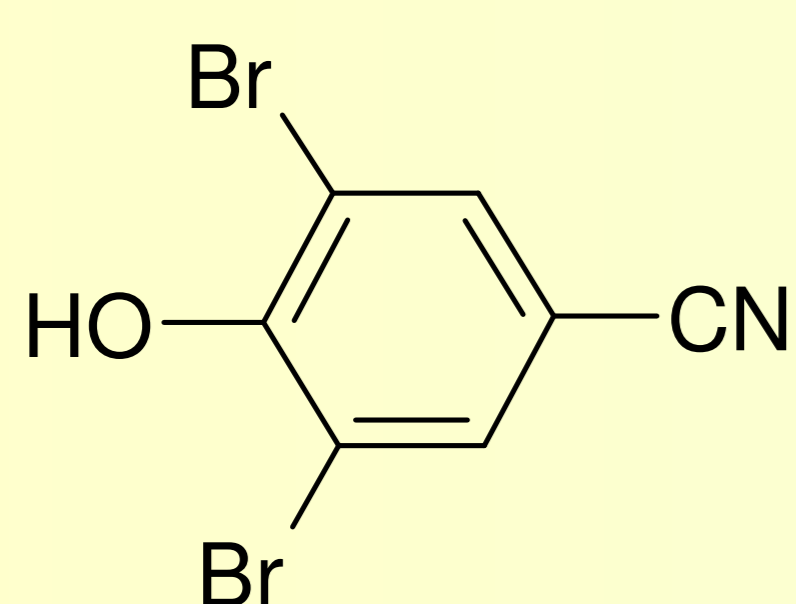


$$F = m \cdot \frac{V}{A}$$

m = Slope
V = Sample volume (cuvette test)
A = TLC application area

For example:
V = 500 µl; A = 0.12 cm²

Application example: Investigation of UV oxidation by-products

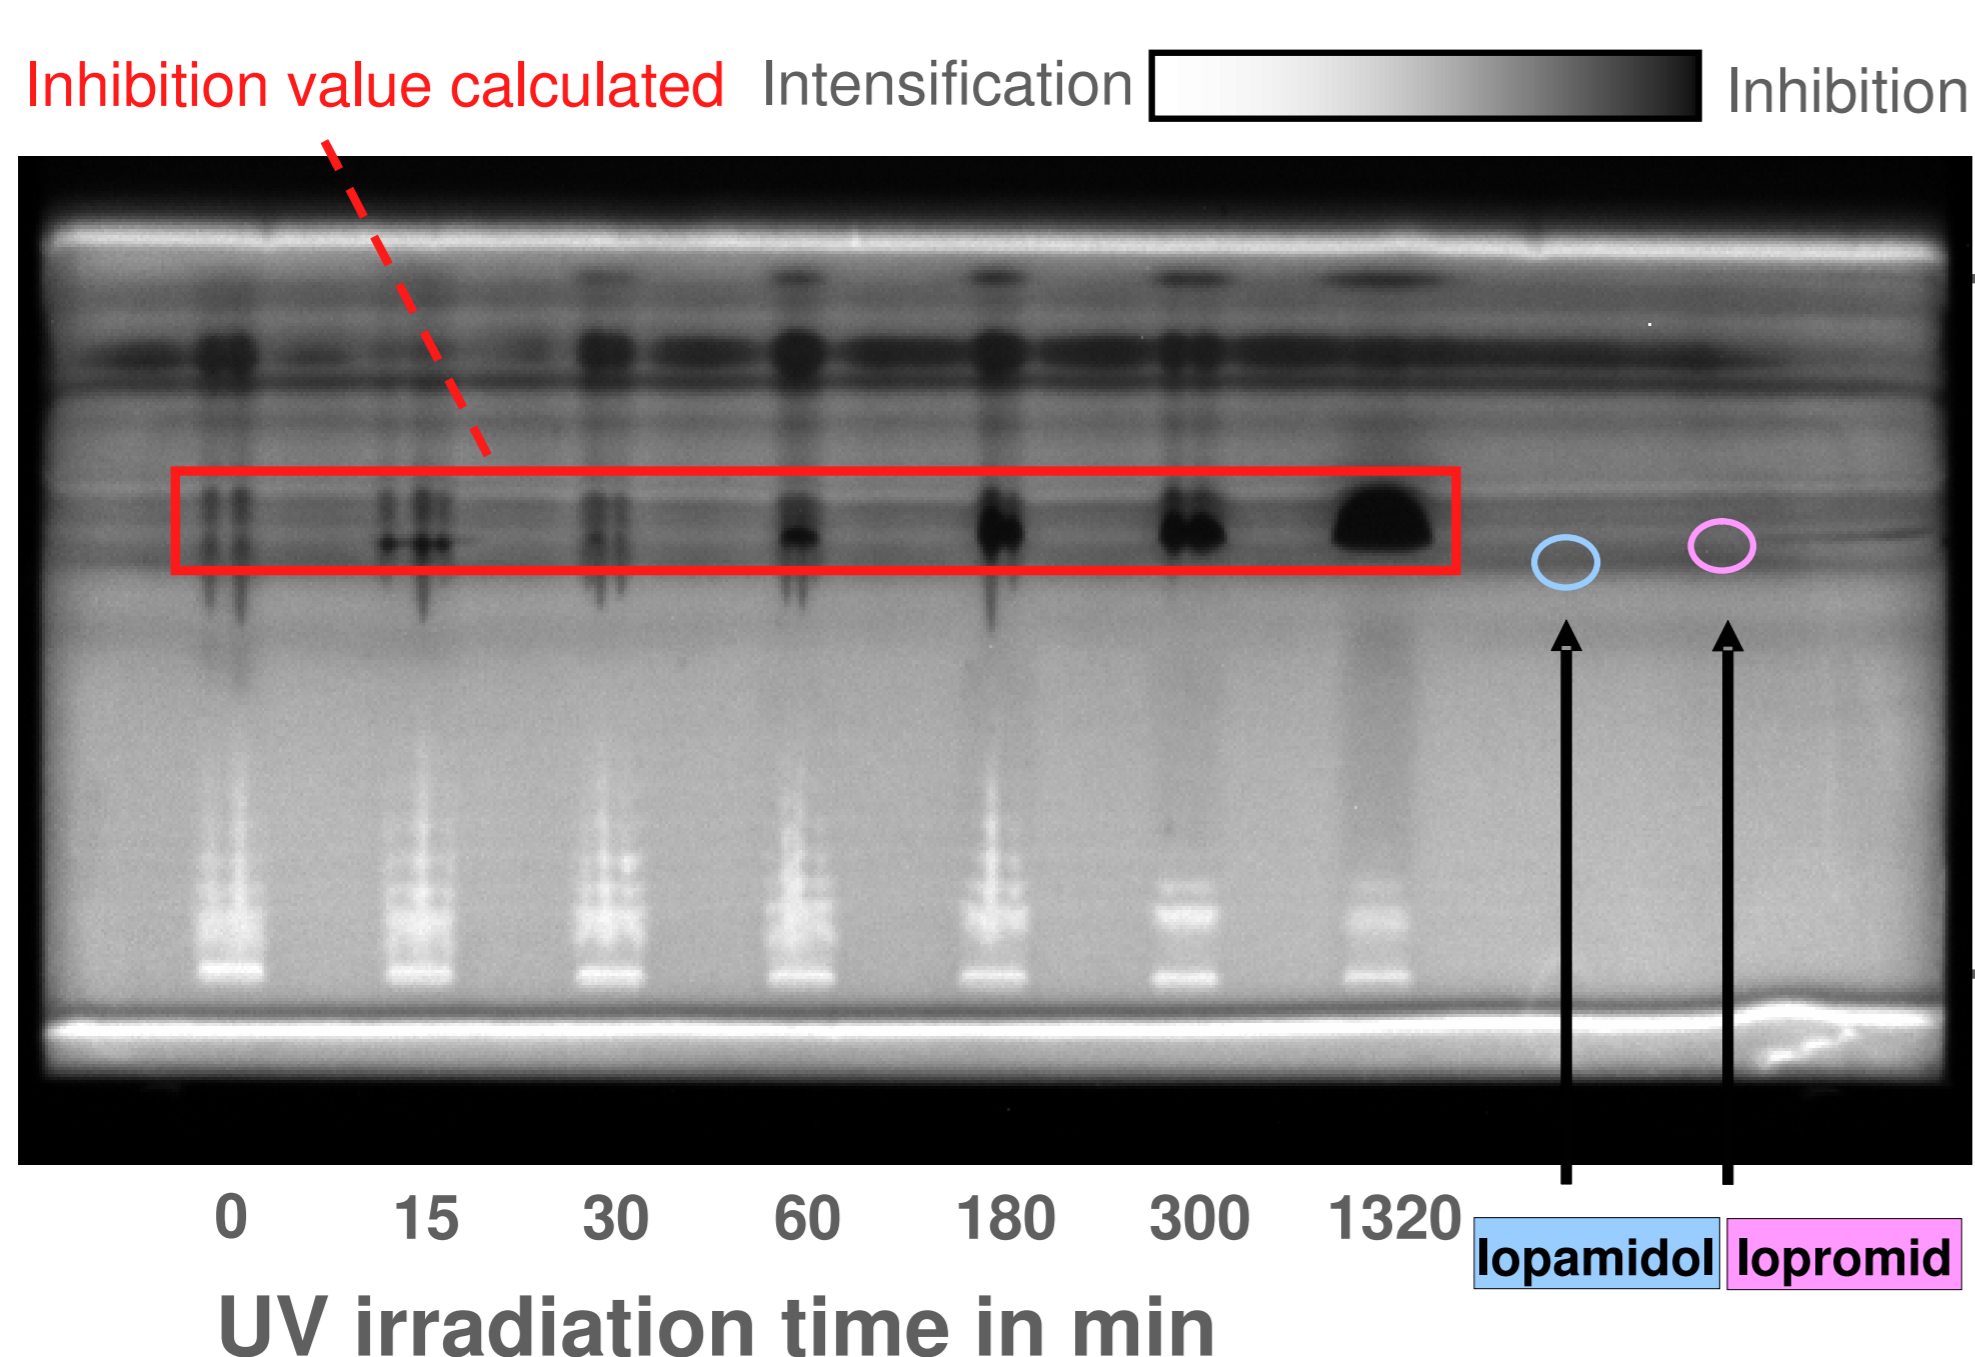

Treatment of X-ray contrast media process waste water by UV irradiation

Luminescence inhibition test on TLC plates

